

Additional Definitions

1910.1030(b)

- *Engineering Controls* - includes additional definitions and examples:

*Sharps with Engineered Sharps
Injury Protections* - [SESIP]


- Non-needle sharp or a needle with a built-in safety feature or mechanism that effectively reduces the risk of an exposure incident

Needleless Systems


Hypodermic syringes with “Self-Sheathing” safety feature




Self-sheathed protected position

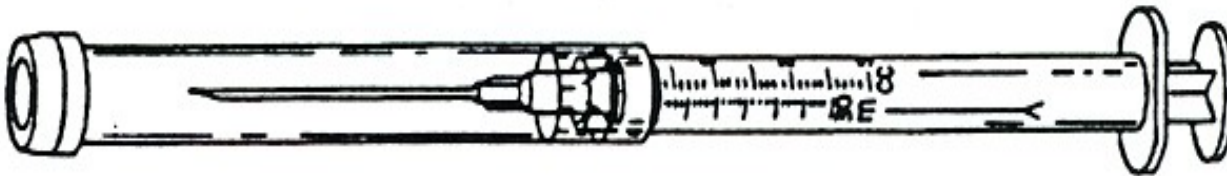


Hypodermic syringes with "Retractable Technology" safety feature

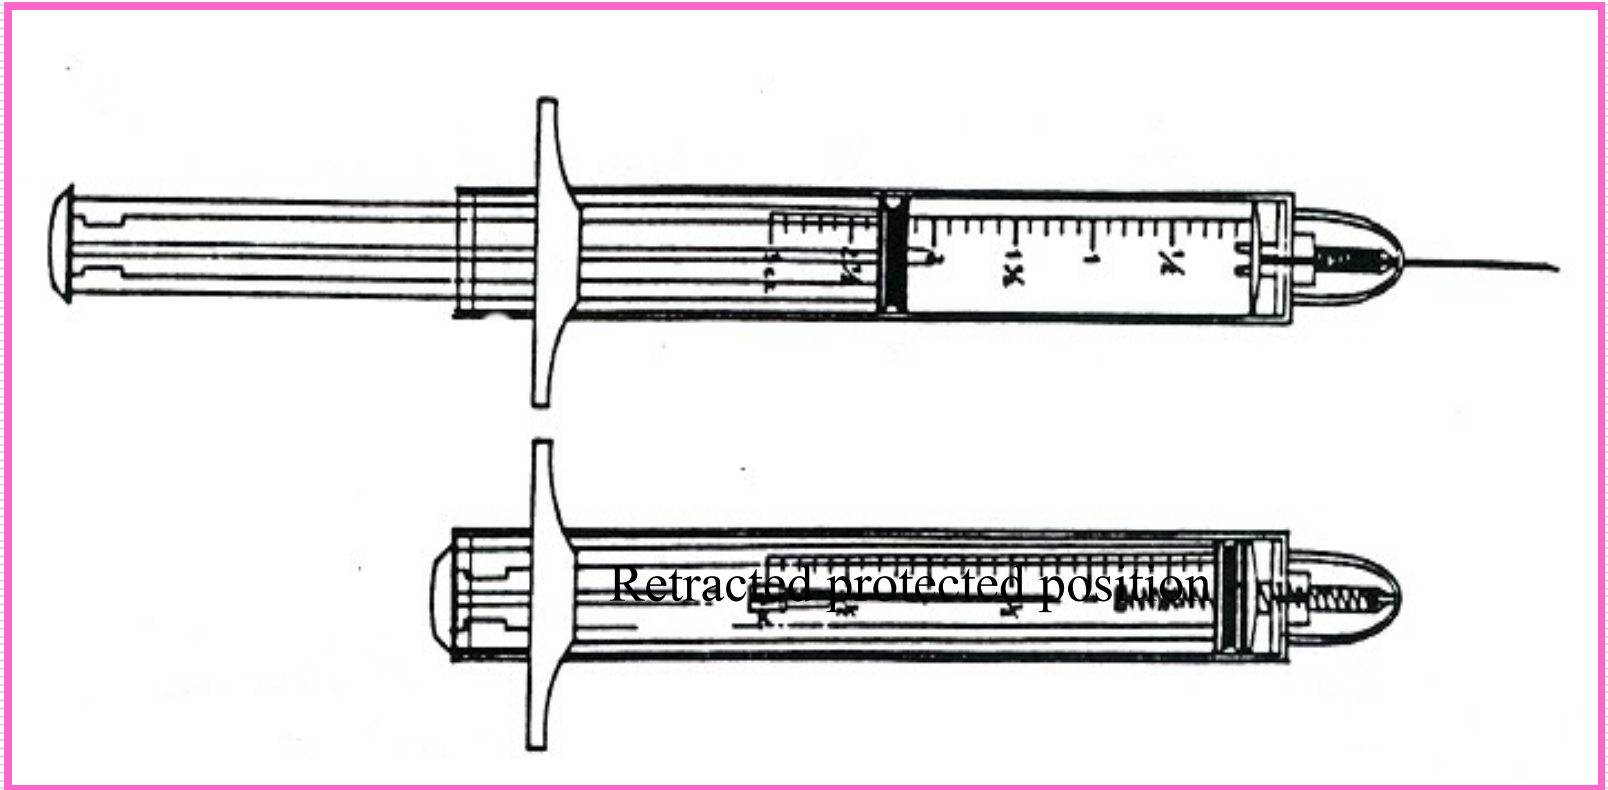



Phlebotomy needle with “Self-Blunting” safety feature

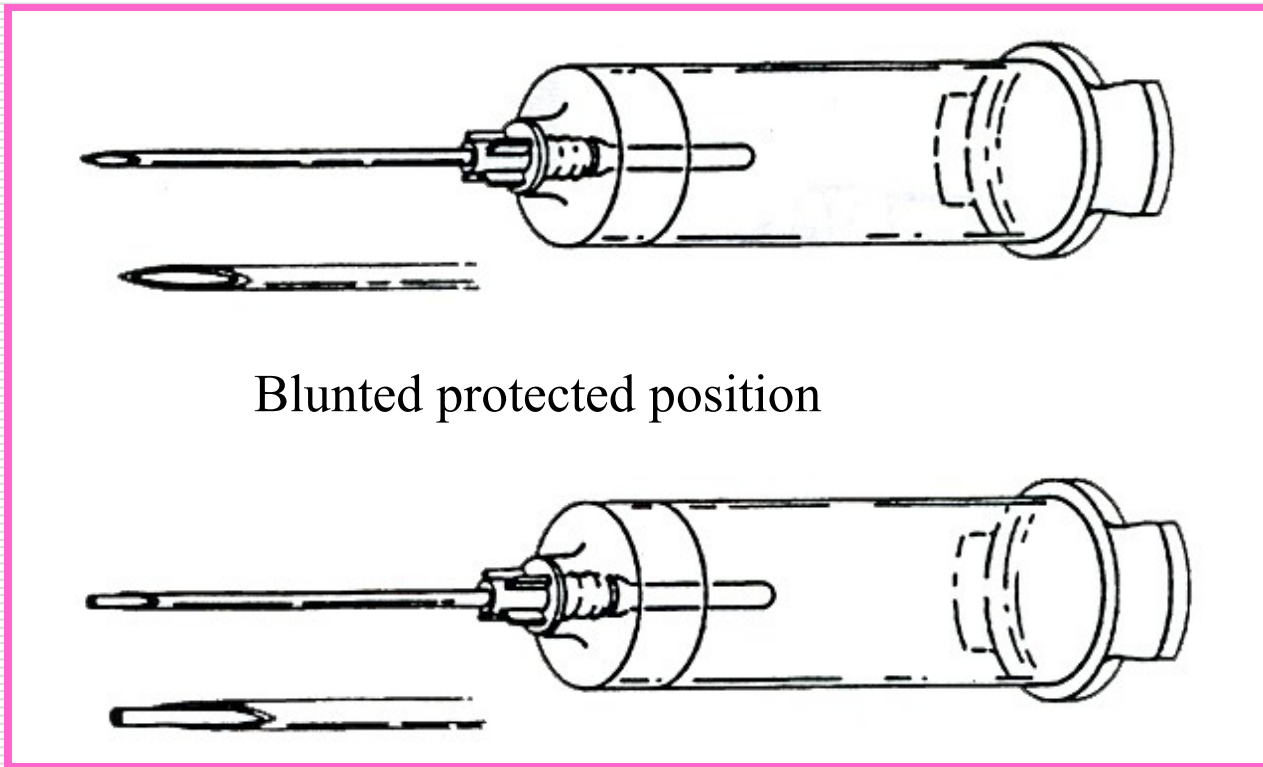


"Add-on" safety feature

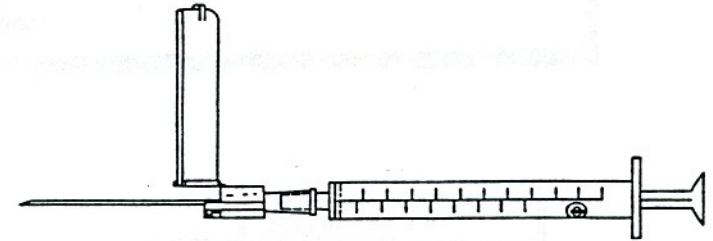


Attached to syringe needle

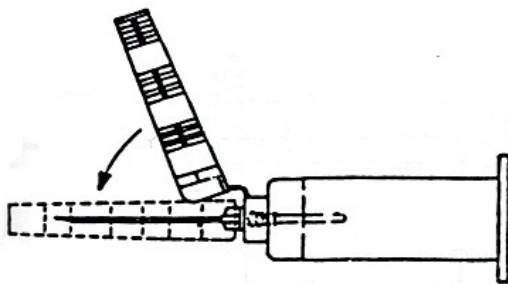


Attached to blood tube holder

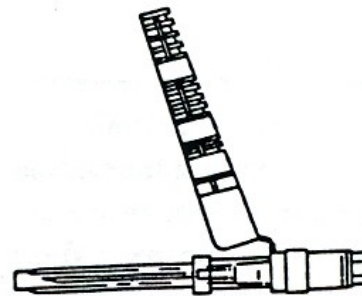


Retracting lancets with safety features.

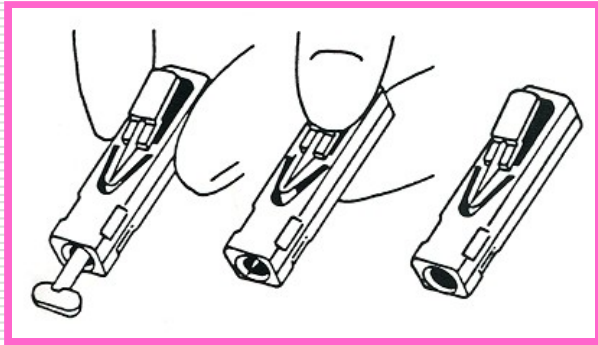

Before During
After

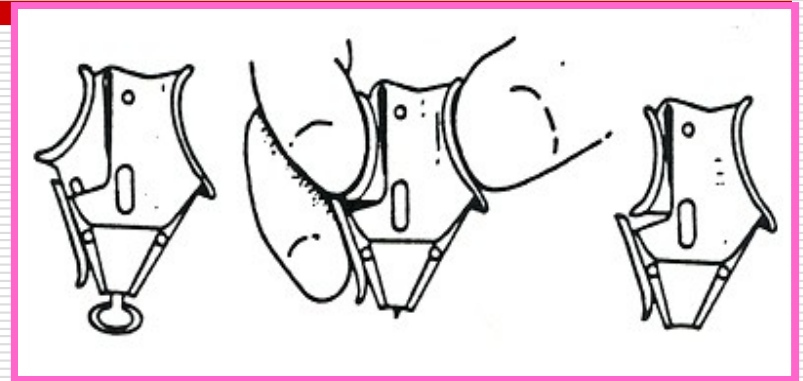


Before During After

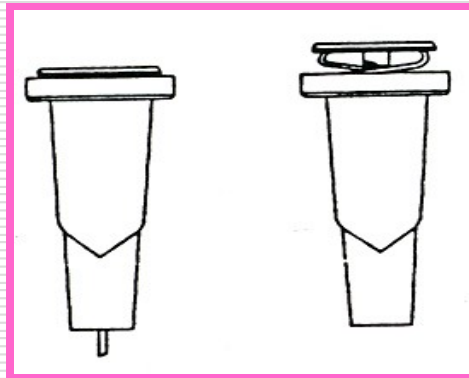


In use After use


Disposable scalpels with safety features.

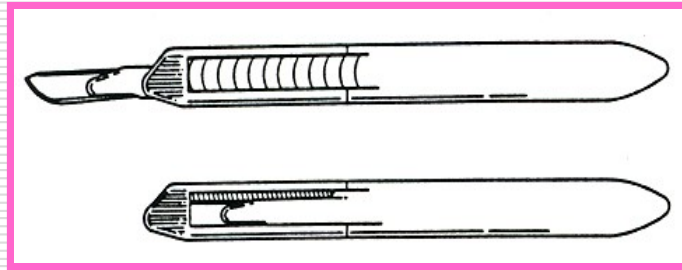

Retracted position

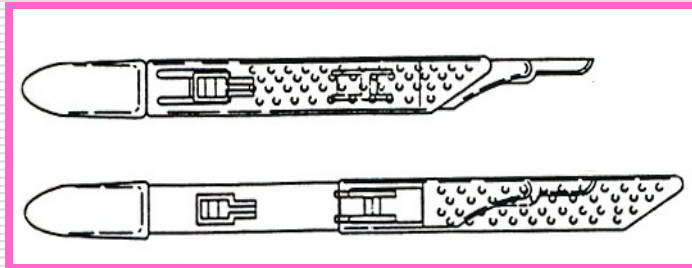

Protracted position

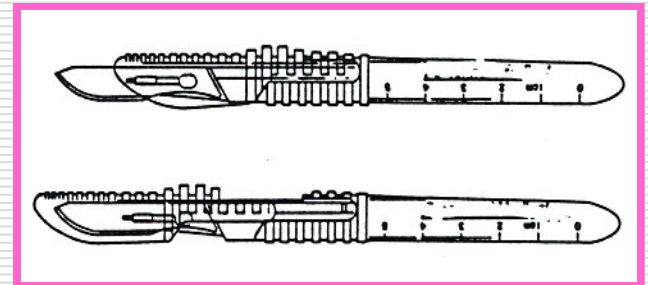

Protracted position

Exposure Control Plan: 1910.1030© - (New Provisions)

The ECP must be updated to include:

- ❑ changes in technology that reduce/eliminate exposure
 - ❑ annual documentation of consideration and implementation of safer medical devices
 - ❑ solicitation of input from non-managerial employees
-